

An Optimizing Dynamic Spectrum Differential Extraction Method for Noninvasive Blood Component Analysis

Wei Tang,^{1,2,3} Qiang Chen,³ Wenjuan Yan,⁴ Guoquan He,⁴ Gang Li,^{1,2} and Ling Lin^{1,*}

¹ State Key Laboratory of Precision Measurement Technology and Instrument, Tianjin University, Tianjin 300072

² China and Tianjin Key Laboratory of Biomedical Detecting Techniques and Instruments, Tianjin University, Tianjin 300072, China

³ The Department of Biomedical Engineering, Hefei University of Technology, Hefei 230009, China

⁴ School of Electronic Information Engineering, Yangtze Normal University, Chongqing 408100, China

*linling@tju.edu.cn

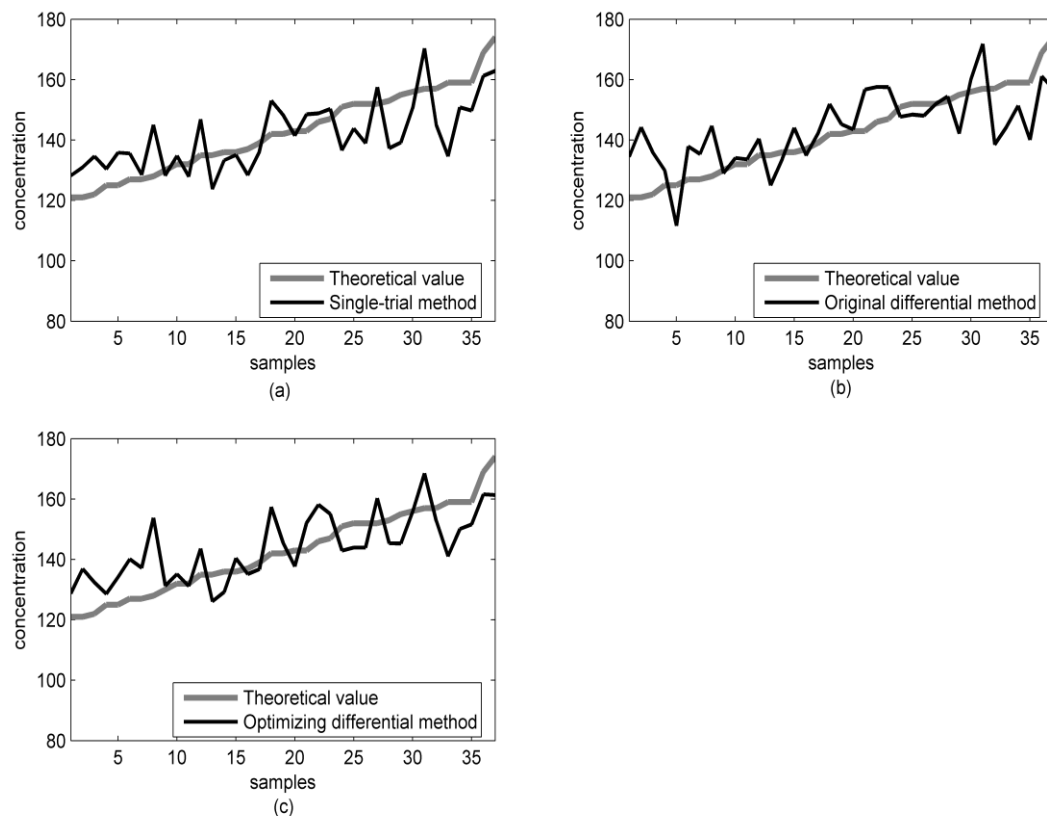


Fig. S1. Neural network modeling effect of prediction set of the three extraction methods (a) Single-trial extraction method. (b) Original differential extraction method. (c) Optimizing differential extraction method.